

Megazyme

www.megazyme.com

HYDROGEN PEROXIDE (MEGAPLEX RED)

ASSAY PROCEDURE

K-MRH2O2 04/21

(1000 Microplate Assays per Kit) or
(100 Manual Assays per Kit) or
(400 Auto-analyser Assays per Kit)



CONTENTS:

INTRODUCTION	1
PRINCIPLE	1
SENSITIVITY, LINEARITY AND PRECISION	1
INTERFERENCE	2
SAFETY	2
KITS	2
PREPARATION OF REAGENT SOLUTIONS/SUSPENSIONS	3
PREPARATION OF WORKING SOLUTION	3
EQUIPMENT (RECOMMENDED)	4
A. MICROPLATE ASSAY PROCEDURE (FLUORESCENCE)	4
PREPARATION OF H ₂ O ₂ CALIBRATION CURVE	4
ASSAY PROCEDURE	5
CALCULATION	5
B. MICROPLATE ASSAY PROCEDURE (ABSORBANCE)	7
PREPARATION OF H ₂ O ₂ STANDARD	7
ASSAY PROCEDURE	7
CALCULATION	8
C. MANUAL ASSAY PROCEDURE (ABSORBANCE)	9
ASSAY PROCEDURE	9
CALCULATION	9
D. AUTO-ANALYSER ASSAY PROCEDURE	11
SAMPLE PREPARATION	12
1. FLUORESCENCE MODE	12
2. ABSORBANCE MODE	12
APPENDIX	13
A. ASSAY PRINCIPLE	13
B. LINEAR RANGE OF ASSAY	13
C. PRECISION OF THE ASSAY	15

INTRODUCTION:

Hydrogen peroxide (H_2O_2) is the simplest peroxide (a chemical with an oxygen-oxygen single bond). H_2O_2 is used as a chemical intermediate, as a bleaching agent in the paper and pulp and textile industries, to sanitise milk handling equipment in dairy industries and in water treatment operations.

Megaplex Red (also known as 10-acetyl-3,7-dihydroxyphenoxazine) is a highly sensitive and stable probe for H_2O_2 . In the presence of horseradish peroxidase (HRP), Megaplex Red reacts with hydrogen peroxide to produce the red-fluorescent oxidation product, resorufin. Resorufin has a fluorometric (excitation and emission maxima of 571 and 585 nm respectively) and colourimetric (absorbance maximum at ~ 570 nm) signal allowing for the use of both fluorometric and colourimetric detection methods.

The Megazyme Hydrogen Peroxide Assay Kit (Megaplex Red) (**K-MRH2O2**) is a simple, user friendly method capable of detecting H_2O_2 in various samples. This kit can also be used to measure enzymatic activity in oxidase-mediated reactions that produce H_2O_2 (subject to end user development).

PRINCIPLE:

The H_2O_2 quantification assay is based on the HRP mediated oxidation of Megaplex Red. Briefly, in the presence of HRP and H_2O_2 the colourless Megaplex red probe is oxidised in a 1:1 stoichiometry to a coloured product (resorufin) that can be measured using a fluorometer equipped for excitation in the range of 530-560 nm and emission at ~ 590 nm or using a spectrophotometer set at 570 nm. H_2O_2 in the sample is then quantified using a calibration curve in fluorescence mode or a single-point standard of known H_2O_2 concentration in absorbance mode.



This principle is shown in more detail in Figure 1 (page 13).

SENSITIVITY, LINEARITY AND PRECISION:

In fluorescence mode, the detection limit is 0.0034 $\mu\text{g/mL}$. As fluorescence values may vary greatly between instruments, the limit of detection is calculated using the lowest value from the linear range of the assay in fluorescence mode, using the recommended sample volume of 0.01 mL. The assay is linear over the range of 0.0034-0.17 $\mu\text{g/mL}$ (0.1 to 5 μM) of H_2O_2 per assay in fluorescence mode.

In absorbance mode, the detection limit is 0.25 $\mu\text{g/mL}$, which is derived from an absorbance difference of 0.020 with the maximum sample volume of 0.4 mL. The assay is linear over the range of 0.034-0.68 $\mu\text{g/mL}$ (1 to 20 μM) of H_2O_2 per assay in absorbance mode.

Linearity graphs for both detection methods are shown in Figures 2 and 4 (pages 13 and 14).

A direct comparison of the Megaplex Red H_2O_2 assay to a competitor red-fluorescent oxidation product H_2O_2 assay in fluorescence mode is shown in Figure 3 (page 14). This comparison shows that the Megaplex Red assay is linear over an extended range versus the competitor's red-fluorescent oxidation product assay.

INTERFERENCE:

Interference caused by the sample matrix can be identified by performing recovery experiments, i.e. by adding a known amount of the H_2O_2 standard to the sample in the test. Quantitative recovery of this standard would be expected.

SAFETY:

The general safety measures that apply to all chemical substances should be adhered to.

For more information regarding the safe usage and handling of this product please refer to the associated SDS that is available from the Megazyme website.

KITS:

Kits suitable for performing 1000 assays in microplate format (or 100 assays in manual format or 400 assays in auto-analyser format) are available from Megazyme. The kits contain the full assay method plus:

Bottle 1: Buffer concentrate (20 mL, pH 7.4) plus sodium azide (0.02% w/v) as a preservative.
Stable for > 2 years at 4°C.

Bottle 2: Megaplex Red, lyophilised powder.
Stable for > 2 years below -10°C.

Bottle 3: Dimethyl sulfoxide (DMSO) (0.6 mL).
Stable for > 2 years at room temperature.

Bottle 4: Horseradish peroxidase (HRP) (0.4 mL).
Stable for > 2 years below -10°C.

Bottle 5: Hydrogen peroxide standard solution (~ 3%, 0.5 mL). See individual component label for exact concentration.
Stable for > 2 years; store sealed at 4°C.

PREPARATION OF REAGENT SOLUTIONS/SUSPENSIONS:

1. Visually inspect bottle 1 for crystallisation before use. If the buffer has crystallised, heat to $\sim 40^{\circ}\text{C}$ for 10 min and mix by inversion until redissolved. Dilute the contents of bottle 1 before use by adding 4 mL of buffer to 36 mL of dH_2O (this is the **Assay Buffer**). This is sufficient for ~ 200 microplate or ~ 20 manual assays with an excess for standard and sample dilution.
Stable for > 3 months at 4°C .
2. Tap the vial on a solid surface prior to opening to ensure that all solid falls to the bottom of the tube. Dissolve the contents by adding 0.55 mL of bottle 3 (DMSO) into the vial. Recap the tube and mix thoroughly. This is the **Megaplex Red** solution. Split into aliquots of ~ 0.1 mL before storage to avoid repeated freeze thaw cycles.
Stable for > 2 years below -10°C .
3. Use the contents of bottle 3 as supplied. DMSO has a high freezing point and the contents may freeze if room temperature falls below $\sim 20^{\circ}\text{C}$. Ensure the DMSO is in liquid form before use by warming gently if necessary.
4. Use the contents of bottle 4 as supplied. Store the bottle in an upright position.
Stable for > 2 years below -10°C .
5. **Dilute the H_2O_2 standard before use.** Consult the label of the H_2O_2 standard to determine the exact percentage (% w/v) of the solution prior to dilution, as the concentration may vary by lot. A guide dilution procedure is given in each assay protocol section.

NOTE: The appropriate H_2O_2 standard solution should be tested with every set of assays as it is used in the calculation of H_2O_2 concentration in the sample analysed.

PREPARATION OF WORKING SOLUTION:

Pipette the following into a ~ 13 mL polypropylene tube. This volume is sufficient for ~ 200 microplate assays or ~ 20 manual cuvette assays.

Component	Volume
Assay Buffer	9.825 mL
Megaplex red bottle 3 (HRP)	0.100 mL 0.075 mL
Total volume	10 mL
Mix well. Make fresh on day of use. Do not store.	

EQUIPMENT (RECOMMENDED):

1. Polypropylene tubes (1.5 mL and ~ 20 mL capacity).
2. Microplate suitable for fluorometric detection or disposable plastic cuvettes (1 cm light path, 1.5 mL).
3. Micro-pipettors, e.g. Gilson Pipetman[®] (200 μ L and 1000 μ L).
4. Positive displacement pipettor, e.g. Eppendorf Multipette[®] with 25 mL Combitip[®] [to dispense 1 mL aliquots of bottle 1, concentrated buffer solution].
5. 20 mL graduated cylinder.
6. Fluorometer equipped for ~ 530-560 nm (excitation) and ~ 590 nm (emission) or Spectrophotometer set at 570 nm, and temperature controlled to 25°C.
7. Vortex mixer (e.g. IKA[®] Yellowline Test Tube Shaker TTS2).

A. MICROPLATE ASSAY PROCEDURE (FLUORESCENCE MODE):

NOTE:

For each set of samples analysed a calibration curve must be performed concurrently in fluorescence mode using the same batch of reagents.

PREPARATION OF H₂O₂ CALIBRATION CURVE:

For fluorescence mode, dilute the H₂O₂ standard (bottle 5) to 0.68 μ g/mL (20 μ M). Calculate the required dilution factor based on the exact stock concentration as per the bottle 5 label. This is the “**diluted standard**”. An example of appropriate dilution for a **3% w/v** solution is outlined below.

Example:

Where bottle 5 contains a stated H₂O₂ concentration of 3% w/v, dilute by dispensing 22.7 μ L of bottle 5 into a polypropylene tube. Add 977.3 μ L of Assay Buffer. Mix well by vortexing. Perform a serial dilution by pipetting 10 μ L of this solution into a second polypropylene tube and adding 9.99 mL of Assay Buffer. Mix well by vortexing. This is the **diluted standard** (0.68 μ g/mL H₂O₂).

Prepare the H₂O₂ solutions as described in the table below (standards 1-5, 0.0034-0.17 μ g/mL of H₂O₂ in the assay) for use in the fluorescence assay procedure as described below. Use fresh on day of preparation, these standards cannot be stored for future use.

Pipette into 13 mL polypropylene tubes	STD 1 0.0034 μ g per mL	STD 2 0.034 μ g per mL	STD 3 0.08 μ g per mL	STD 4 0.114 μ g per mL	STD 5 0.17 μ g per mL
Assay Buffer diluted standard	1.47 mL 0.03 mL	1.2 mL 0.3 mL	0.8 mL 0.7 mL	0.5 mL 1.0 mL	- 1.5 mL
total volume	1.5 mL	1.5 mL	1.5 mL	1.5 mL	1.5 mL

ASSAY PROCEDURE:

Detection method:	Fluorescence
Excitation:	530-560 nm
Emission:	~ 590 nm
Microplate:	96-well (e.g. black, flat-bottomed, polystyrene)
Temperature:	~ 25°C
Final volume:	0.10 mL
Linearity:	0.0034-0.17 µg/mL of H ₂ O ₂ per assay (0.1-5 µM in-assay)

Pipette into wells	Blank	Sample	Standard
Assay Buffer	0.050 mL	0.040 mL	0.025 mL
sample	-	0.010 mL	-
standards 1 - 5	-	-	0.025 mL
Mix*, allow the reaction to equilibrate to temperature for 5 min and start the reaction by addition of:			
working solution	0.05 mL	0.05 mL	0.05 mL
Mix* and read the absorbance of the solutions (Abs) after exactly 30 min.			

* for example using microplate shaker, shake function on a microplate reader or repeated aspiration (e.g. using a pipettor set at 50-100 µL volume).

CALCULATION:

1. Determine the average of the duplicate readings for the blank, H₂O₂ standards and samples.
2. Correct for background fluorescence by subtracting the average of the blank values from the H₂O₂ standard values thereby obtaining Standard_{cor}.
3. Plot a calibration curve showing the corrected fluorescence values (Standard_{cor}) on the X-axis against the concentration of H₂O₂ [µg/mL in-assay] on the Y-axis using a suitable software such as Excel. A new calibration curve must be completed for each assay.
4. Calculate the linear trendline and the equation of the line based on your calibration curve data.
5. Correct for background fluorescence in the samples of interest by subtracting the average of the blank values from the average sample values thereby obtaining Sample_{cor}.
6. Extrapolate the concentration of the corrected sample using the following equation;

$$y = \text{Slope (m)} \times \text{Sample}_{\text{cor}} + b \quad [\mu\text{g/mL in-assay}]$$

The concentration of H₂O₂ in the sample is calculated as follows:

$$c = \frac{y \times 0.1 \times F}{0.01} \quad [\mu\text{g/mL}]$$

where:

- y** = $\mu\text{g/mL}$ in-assay calculated from the standard curve
0.1 = total assay volume [mL]
F = dilution of sample
0.01 = sample volume in-assay [mL]

The content of H₂O₂ in μM can then be calculated, if required, as follows:

$$c = \mu\text{g/mL} \times 1000 \times \frac{1}{34.015} \quad [\mu\text{M}]$$

where:

- $\mu\text{g/mL}$ = concentration of H₂O₂ in the sample
1000 = conversion from mL to L
34.015 = Molecular weight of H₂O₂ in g/mol

NOTE: These calculations can be simplified by using the Megazyme **Mega-Calc**TM, downloadable from where the product appears in the Megazyme web site (www.megazyme.com).

Example:

The linear trendline for the sample data in Figure 1 (Page 13) of this assay protocol gives the following equation:

$$y = 0.0004x - 0.0005 \quad (\text{in the form } y = mx + b)$$

If the Sample_{cor} value in this analysis is 300 RFU for an undiluted sample then the concentration of H₂O₂ in the assay can be calculated as follows:

$$y = 0.0004 \times 300 - 0.0005 = 0.1195 \mu\text{g/mL in-assay}$$

The concentration of H₂O₂ in the sample is calculated as follows:

$$c = \frac{0.1195 \times 0.1 \times 1}{0.01} = 1.195 \mu\text{g/mL}$$

The content of H₂O₂ in μM can then be calculated, if required, as follows:

$$c = 1.195 \times 1000 \times \frac{1}{34.015} = 35.13 \mu\text{M}$$

NOTE: These calculations can be simplified by using the Megazyme **Mega-Calc™**, downloadable from where the product appears in the Megazyme web site (www.megazyme.com).

B. MICROPLATE ASSAY PROCEDURE (ABSORBANCE MODE):

PREPARATION OF H₂O₂ STANDARD:

For absorbance mode, prepare a single point standard by diluting the H₂O₂ standard (bottle 5) to 6.8 µg/mL (200 µM). Calculate the required dilution factor based on the exact stock concentration as per the bottle 5 label. This is the “**diluted standard**”. An example of an appropriate dilution for a **3% w/v** solution is outlined below.

Example:

Where bottle 5 contains a stated H₂O₂ concentration of 3% w/v dilute by dispensing 22.7 µL of bottle 5 into a polypropylene tube. Add 977.3 µL of Assay Buffer. Mix well by vortexing. Perform a serial dilution by pipetting 10 µL of this solution into a second polypropylene tube and adding 990 µL of Assay Buffer. Mix well by vortexing. This is the **diluted standard** (6.8 µg/mL H₂O₂).

ASSAY PROCEDURE:

Detection method: Absorbance
Wavelength: 570 nm
Microplate: 96-well (e.g. clear flat-bottomed, glass or plastic)
Temperature: ~ 25°C
Final volume: 0.10 mL
Linearity: 0.03-0.68 µg/mL of H₂O₂ per assay
(1-20 µM in-assay)

Pipette into cuvettes	Blank	Sample	Standard
Assay Buffer	0.050 mL	0.040 mL	0.045 mL
sample	-	0.010 mL	-
diluted standard	-	-	0.005 mL
Mix*, allow the reaction to equilibrate to temperature for 5 min and start the reaction by addition of:			
working solution	0.05 mL	0.05 mL	0.05 mL
Mix* and read the absorbance of the solutions (A ₁) at the end of the reaction (~ 10 min).			

* the sample volume in the test can be increased to 0.04 mL if an increase in sensitivity is required. If the sample volume is increased, the volume of solution I (Assay Buffer) should be reduced proportionately.

** for example using microplate shaker, shake function on a microplate reader or repeated aspiration (e.g. using a pipette set at 50-100 µL volume).

CALCULATION:

Determine the absorbance difference between the absorbance of the standard and of the blank ($Abs_{\text{standard}} - Abs_{\text{blank}}$) after 30 min, thereby obtaining $\Delta Abs_{\text{standard}}$.

Calculate **M** as follows:

$$M = \frac{H_2O_2 \text{ (}\mu\text{g/mL in-assay)}}{\Delta Abs_{\text{standard}}}$$

Determine the absorbance difference between the absorbance of the sample and of the blank ($Abs_{\text{sample}} - Abs_{\text{blank}}$) after 30 min, thereby obtaining $\Delta Abs_{\text{sample}}$.

The concentration of H_2O_2 can then be calculated as follows:

$$c = \Delta Abs_{\text{sample}} \times M \times \frac{V_1}{V_2} \times F \quad [\mu\text{g/mL}]$$

where:

$$\Delta Abs_{\text{sample}} = Abs_{\text{sample}} - Abs_{\text{blank}}$$

$$M = \text{value of } H_2O_2 \text{ standard } [\mu\text{g}/\Delta Abs_{\text{standard}}]$$

$$V_1 = \text{total assay volume [mL]}$$

$$F = \text{dilution of sample}$$

$$V_2 = \text{sample volume in assay [mL]}$$

The content of H_2O_2 in μM can then be calculated, if required, as follows:

$$c = \mu\text{g/mL} \times 1000 \times \frac{1}{34.015} \quad [\mu\text{M}]$$

where:

$$\mu\text{g/mL} = \text{concentration of } H_2O_2 \text{ in the sample}$$

$$1000 = \text{conversion from mL to L}$$

$$34.015 = \text{Molecular weight of } H_2O_2 \text{ in g/mol}$$

Example:

Where the 6.8 $\mu\text{g/mL}$ diluted standard is prepared as described in the assay procedure and 0.005 mL of this is used in a final assay volume of 0.1 mL the amount of H_2O_2 in assay is 0.34 $\mu\text{g/mL}$. If, for example, the $\Delta Abs_{\text{standard}}$ measured in the assay is 0.650, then the “M” value can be calculated as follows:

$$M = \frac{0.34}{0.650} = 0.52$$

If the $\Delta Abs_{\text{sample}}$ measured in the assay for an undiluted sample is 0.700 then the concentration of H_2O_2 is calculated as follows:

$$c = 0.700 \times 0.52 \times \frac{0.1}{0.01} \times 1 = 3.64 \mu\text{g/mL}$$

The content of H₂O₂ in μM can then be calculated, if required, as follows:

$$c = 3.64 \times 1000 \times \frac{1}{34.015} = 107 \mu\text{M}$$

NOTE: These calculations can be simplified by using the Megazyme **Mega-Calc**[™], downloadable from where the product appears in the Megazyme web site (www.megazyme.com).

C. MANUAL ASSAY PROCEDURE (ABSORBANCE MODE):

Prepare a 6.8 μg/mL (200 μM) H₂O₂ diluted standard solution as described on page 7 in this assay protocol.

ASSAY PROCEDURE:

Detection method: Absorbance

Wavelength: 570 nm

Cuvette: 1 cm light path (glass or plastic)

Temperature: 25°C

Final volume: 1.0 mL

Sample solution: 0.034-0.68 μg/mL of H₂O₂ per assay
(1-20 μM in-assay)

Read against air (without a cuvette in the light path) or against water

Pipette into cuvettes	Blank	Sample	Standard
assay buffer	0.50 mL	0.40 mL	0.45 mL
sample	-	0.10 mL*	-
diluted standard	-	-	0.05 mL
Mix*, allow the reaction to equilibrate to temperature for 5 min and start the reaction by addition of:			
working solution	0.50 mL	0.50 mL	0.50 mL
Mix** and read the absorbance of the solutions (Abs) after exactly 15 min.			

* the sample volume in the test can be increased to 0.4 mL if an increase in sensitivity is required. If the sample volume is increased, the volume of solution I (Assay Buffer) should be reduced proportionately.

** for example with a plastic spatula or by gentle inversion after sealing the cuvette with a cuvette cap or Parafilm[®].

CALCULATION:

Determine the absorbance difference between the absorbance of the standard and of the blank (Abs_{standard} - Abs_{blank}) after 30 min, thereby obtaining ΔAbs_{standard}.

Calculate **M** as follows:

$$\mathbf{M} = \frac{\text{H}_2\text{O}_2 \text{ (}\mu\text{g/mL in-assay)}}{\Delta\text{Abs}_{\text{standard}}}$$

Determine the absorbance difference between the absorbance of the sample and of the blank ($\text{Abs}_{\text{sample}} - \text{Abs}_{\text{blank}}$) after 30 min, thereby obtaining $\Delta\text{Abs}_{\text{sample}}$.

The concentration of H_2O_2 can then be calculated as follows:

$$\mathbf{c} = \Delta\text{Abs}_{\text{sample}} \times \mathbf{M} \times \frac{V_1}{V_2} \times \mathbf{F} \quad [\mu\text{g/mL}]$$

where:

$$\Delta\text{Abs}_{\text{sample}} = \text{Abs}_{\text{sample}} - \text{Abs}_{\text{blank}}$$

$$\mathbf{M} = \text{value of } \text{H}_2\text{O}_2 \text{ standard } [\mu\text{g}/\Delta\text{Abs}_{\text{standard}}]$$

$$V_1 = \text{total assay volume [mL]}$$

$$\mathbf{F} = \text{dilution of sample}$$

$$V_2 = \text{sample volume in assay [mL]}$$

The content of H_2O_2 in μM can then be calculated, if required, as follows:

$$\mathbf{c} = \mu\text{g/mL} \times 1000 \times \frac{1}{34.015} \quad [\mu\text{M}]$$

where:

$$\mu\text{g/mL} = \text{concentration of } \text{H}_2\text{O}_2 \text{ in the sample}$$

$$1000 = \text{conversion from mL to L}$$

$$34.015 = \text{Molecular weight of } \text{H}_2\text{O}_2 \text{ in g/mol}$$

Example:

Where the 6.8 $\mu\text{g/mL}$ diluted standard is prepared as described in the assay procedure and 0.05 mL of this is used in the assay the amount of H_2O_2 in assay is 0.34 $\mu\text{g/mL}$. If, for example, the $\Delta\text{Abs}_{\text{standard}}$ measured in the assay is 0.650, then the “M” value can be calculated as follows:

$$\mathbf{M} = \frac{0.34}{0.650} = 0.52$$

If the $\Delta\text{Abs}_{\text{sample}}$ measured in the assay for an undiluted sample is 0.700 then the concentration of H_2O_2 is calculated as follows:

$$c = 0.700 \times 0.52 \times \frac{1.0}{0.1} \times 1 = 3.64 \mu\text{g/mL}$$

The content of H_2O_2 in μM can then be calculated, if required, as follows:

$$c = 3.64 \times 1000 \times \frac{1}{34.015} = 107 \mu\text{M}$$

NOTE: These calculations can be simplified by using the Megazyme *Mega-Calc*TM, downloadable from where the product appears in the Megazyme web site (www.megazyme.com).

D. AUTO-ANALYSER ASSAY PROCEDURE:

NOTE:

For each set of samples tested in the Auto-Analyser format either a single point standard or a calibration curve must be performed concurrently using the same batch of reagents.

Reagent preparation for ~ 100 assays is performed as follows:

R1: Assay buffer, 10 mL (see preparation, page 3)

R2: Working solution, 10 mL (see preparation, page 3)

H₂O₂ standard: Prepare a diluted H₂O₂ standard as described on page 7 in this assay protocol.

EXAMPLE METHOD:

R1: 0.1 mL

Sample: 0.025 mL

R2: 0.125 mL

Reaction time: 30 min at 25°C

Wavelength: 570 nm

Prepared reagent stability: R1 is stable for ~ 3 months stored at 4°C. Prepare R2 and H₂O₂ standard freshly on the day of assay.

Reaction direction: Increase

Linearity: up to 9.0 μg/mL of H₂O₂ using 0.025 mL sample volume

SAMPLE PREPARATION:

Fluorescence mode:

In fluorescence mode, the amount of H_2O_2 present in the test should range between 0.00034-0.017 μg per assay (0.1-5 μM in-assay concentration). The original sample solution must therefore be diluted sufficiently to yield a H_2O_2 concentration between 0.034-1.7 $\mu\text{g}/\text{mL}$ (1-50 μM) when using the recommended assay volume of 0.01 mL. In order to achieve sufficiently accurate results the value for the sample in relative fluorescence units (RFU) should not exceed the value achieved for STD 5 (0.17 $\mu\text{g}/\text{mL}$ in-assay) in the calibration curve. Recommended dilutions of sample are described in the table below.

H_2O_2 ($\mu\text{g}/\text{mL}$)	H_2O_2 (μM)	Dilution with dH_2O	Dilution factor (F)
< 1.7	< 100	No dilution	1
1.7-17	100-1000	1 + 9	10
17-170	1000-10,000	1 + 99	100
> 170	> 10,000	1 + 999	1000

If the RFU value is lower than STD 1 (0.0034 $\mu\text{g}/\text{mL}$ in-assay) in the calibration curve, weigh out more sample or dilute less strongly.

Absorbance mode:

In absorbance mode (microplate), the amount of H_2O_2 present in the test (i.e. in the 0.01 mL of sample being analysed) should range between 0.003-0.068 μg per assay (1-20 μM in-assay concentration). In absorbance mode (manual) the amount of H_2O_2 present in the test (i.e. in the 0.1 mL of sample being analysed) should range between 0.034-0.68 μg per assay (1-20 μM in-assay concentration). The original sample solution must therefore be diluted sufficiently to yield a H_2O_2 concentration between 0.34-6.8 $\mu\text{g}/\text{mL}$ (10-200 μM) before analysis. In order to achieve sufficiently accurate results, the value of $\Delta\text{Abs}_{\text{sample}}$ should as a rule be at least 0.1 absorbance units and not more than 2.0 absorbance units in absorbance mode. Recommended dilutions of sample are described in the table below.

H_2O_2 ($\mu\text{g}/\text{mL}$)	H_2O_2 (μM)	Dilution with dH_2O	Dilution factor (F)
< 6.8	< 0.5	No dilution	1
6.8-68	0.5-5	1 + 9	10
68-680	5-50	1 + 99	100
> 680	> 50	1 + 999	1000

If the value of $\text{Abs}_{\text{sample}}$ is too low (e.g. < 0.1), weigh out more sample or dilute less strongly.

APPENDIX:

A. Assay Principle - H₂O₂ detection

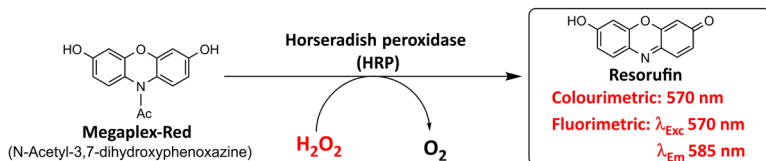


Figure 1. Theoretical basis of the H₂O₂ detection assay.

B. Linear range of assay

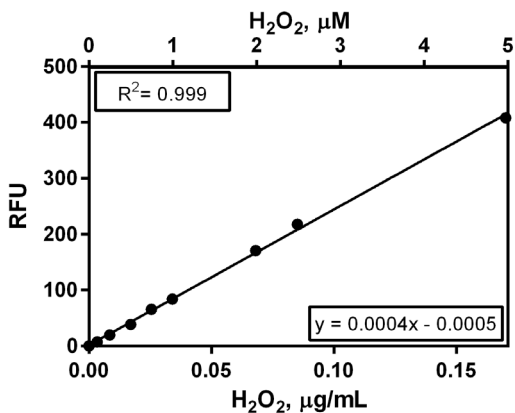


Figure 2. Linearity of the H₂O₂ assay in fluorescence mode. Fluorescence was measured with a fluorescence microplate reader using excitation at 530 nm and emission at 590 nm wavelengths. Note that a new calibration curve must be completed for each batch of samples. This data is provided for demonstrative purposes only.

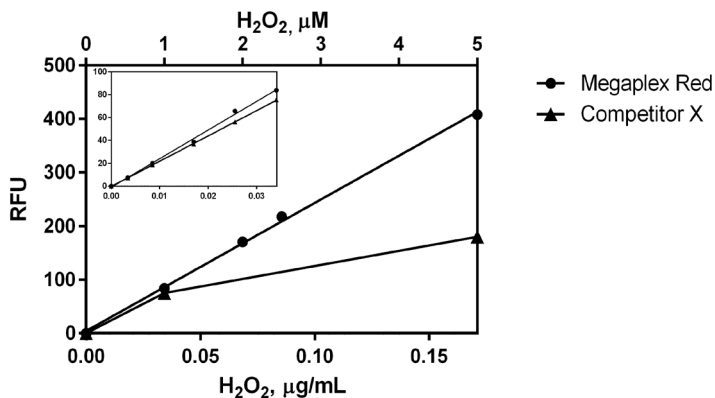


Figure 3. Comparison of linearity of the H₂O₂ assay in fluorescence mode versus a comparable competitor red-fluorescent assay. The Megaplex Red assay is linear over an extended range. Fluorescence was measured with a fluorescence microplate reader using excitation at 530 nm and emission at 590 nm wavelengths.

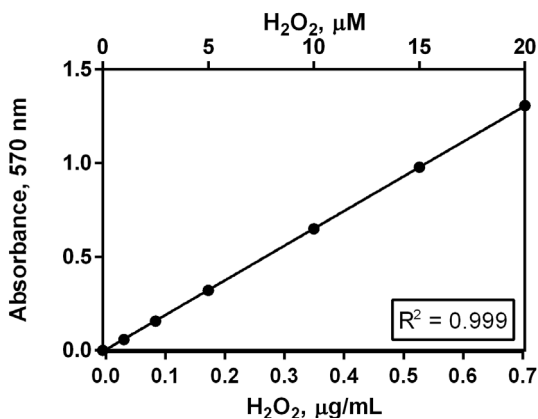


Figure 4. Linearity of the H₂O₂ assay in absorbance mode.

C. Precision of the assay

Analyte	n	$\mu\text{g H}_2\text{O}_2$ per test	Mean, RFU H_2O_2	Standard Deviation	% CV
H_2O_2	10	0.00034	7.142	0.278	3.9
	10	0.0017	35.520	2.970	8.4
	10	0.0034	80.180	6.081	7.6
	10	0.0085	189.944	3.010	1.6
	10	0.0170	381.247	8.415	2.2

Figure 5. Intermediate precision values in microplate fluorescence mode obtained using a range of H_2O_2 standards in the assay kit.

Analyte	n	$\mu\text{g H}_2\text{O}_2$ per test	Mean, Abs H_2O_2	Standard Deviation	% CV
H_2O_2	23	0.170	0.339	0.024	7.2
	24	0.340	0.705	0.043	6.1
	24	0.680	1.413	0.049	3.5

Figure 6 Intermediate precision values in manual absorbance mode obtained using a range of H_2O_2 standards in the assay kit.



**Bray Business Park, Bray,
Co. Wicklow,
A98 YV29,
IRELAND.**

**Telephone: (353.1) 286 1220
Facsimile: (353.1) 286 1264
Internet: www.megazyme.com
E-Mail: info@megazyme.com**

WITHOUT GUARANTEE

The information contained in this assay protocol is, to the best of our knowledge, true and accurate, but since the conditions of use are beyond our control, no warranty is given or is implied in respect of any recommendation or suggestions which may be made or that any use will not infringe any patents.