



Dynamic Test Kits for R&D
and Quality Control

ABTS Assay Kit

KF-01-002

250 tests (96 well plate)

BOCKit

A brand of  **Bio
QuoChem**

Votre interlocuteur en France, Belgique, Luxembourg et Suisse :

LIBIOS

83, rue Edmond Michelet - 69490 Pontcharra Sur Turdine - France

Tél. : +33 (0)4 74 13 03 02 - Fax : +33 (0)4 74 05 28 25 –

Mail : info@libios.fr - www.libios.fr

Index

Introduction	Pag. 1
Materials	Pag. 2
Assay Principle	Pag. 3
Reagent Preparation	Pag. 4
Assay Protocol	Pag. 5
Data Analysis	Pag. 8
Warranties and Limitation of Liability	Pag. 10



All chemicals should be handled with

- This kit is for R&D use only

Introduction

Antioxidant capacity is an overall ability of organisms or food to catch free radicals and prevent their harmful effect. Antioxidative effect includes protection of cells and cellular structures against harmful effect of free radicals, especially oxygen and nitrogen. Substances with antioxidative properties are called antioxidants. They are contained in food and food supplements, most commonly in fruits, vegetables, rice, wine, meat, eggs, and other foodstuff of plant and animal origin.

Antioxidative systems include antioxidative enzymes, that is, superoxide dismutase, catalase, glutathione peroxidase, glutathione-S-transferase, and nonenzymatic substrates, such as glutathione, uric acid, lipoic acid, bilirubin, coenzyme Q, vitamin C (L-ascorbic acid), vitamin A (retinol), vitamin E (tocopherol), flavonoids, carotenoids, teine compounds in green tea, and others. Some biomolecules are also considered biologically active and clinically significant antioxidants, for example, transferrin, ferritin, lactoferrin, ceruloplasmin, hemopexin, haptoglobin, and uric acid.

Materials

BQCKit ABTS Assay Kit KF-01-002 250 tests (96 well plate) contains:

Product	Quantity	Storage
Reagent A	5 vials	-20 °C
Reagent B	1 bottle	RT
Standard	2 vials	RT

Note 1: Each vial of Reagent A is valid for 50 tests. Discard the remaining solution.

Note 2: Each vial of Standard is valid for 125 tests. Discard the remaining solution.


Assay Principle

Bioquochem ABTS assay kit is recommended for total antioxidant activity of solutions of pure substances, aqueous mixtures and beverages.

The assay described here involves the direct production of the blue/green ABTS^{•+} chromophore. This has absorption maxima at 734 nm.

The addition of antioxidants to the pre-formed radical cation, reduces it ABTS depending on the antioxidant activity and the concentration of the antioxidant.

In our assay a solution of ABTS at neutral pH and in the presence of a suitable solution, can form a stable and colored radical cation (ABTS^{•+}) which shows a maximum of absorbance at 734 nm. Antioxidant compounds quench the color and produce a decoloration of the solution which is proportional to their amount. This reaction is rapid and the end, which is stable, is taken as a measure of the antioxidative efficiency.

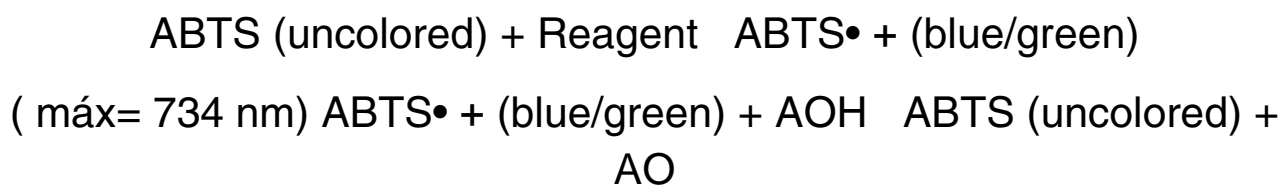

Scheme 1. Formation of radical ABTS and its reaction with antioxidants (AOH)

Reagent Preparation

Allow the reagents to reach room temperature.

ABTS Solution:

For each 50 tests, dilute Reagent A with Reagent B in a 10 ml tube (not provided), to an absorbance of around **0.70** (± 0.02) at 734 nm.

This value is obtained with a dilution between 1:40 and 1:50 of Reagent A with Reagent B .

This solution is called ABTS Solution. Use this solution immediately.

Standard solutions:

For standard solution preparation, add exactly 1 mL of deionized water to each Standard vial. This solution must be freshly prepared.

Dilute 1:10 the Standard Solution previously prepared.

Samples:

Dilute your sample in EtOH (for phenolic compounds and food extracts) or ddH₂O (for plasma) such that, after introduction of 5 μ L of each aliquot into 200 μ L of ABTS Solution, it produces between 5%-35% inhibition of the blank absorbance (ABTS• + alone).

Assay Protocol

Standard Calibration Curve

Prepare calibration curves in 1.5 mL tubes as shown in Table 1.

NOTE: Keep these tubes in ice during the assay.

Table 1. Reagent volumes needed to carry out the standard curve

	ddH ₂ O [μL]	Standard [μL]	CEAC* [μM]
S1 (Blank)	100	0	0
S2	90	10	100
S3	85	15	150
S4	75	25	250
S5	70	30	300
S6	60	40	400
S7	50	50	500
S8	40	60	600

*Antioxidant activity is expressed as CEAC (Vitamin C equivalents antioxidant capacity).

Assay Protocol

Plate set up

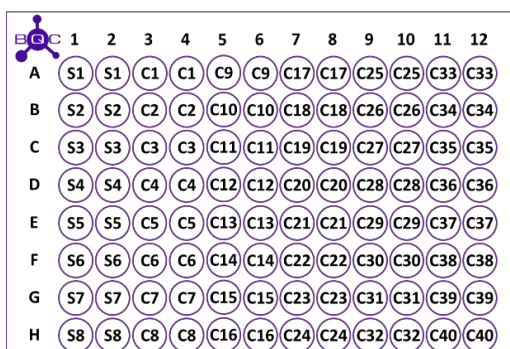


Figure 1. 96-well plate filling format

S1-S8: Standards

C1-C40 = Samples


Attention

- This scheme is just a recommendation of how to perform the assay.
 - If the antioxidant activity in the samples is not known or if it is expected to be beyond the range of the standard curve, it is recommended to assay the samples at several dilutions.
 - For optimal results, it is recommended to run the standards and the samples for duplicate, but it is the user's discretion to do so.
- The blank sample absorbance (A_0) must be 0.7

Assay Protocol

Short protocol:

1



Prepare all reagents and 96 well plate.

2




Add 5 μL of the sample standard in each well.

3



Add 200 μL of ABTS Solution you have previously prepared (see Reagent preparation) in each well.

4



Mix the mixture for 5 minutes under continuous stirring.

5



Read the absorbance at 734 nm at about 27°C.

Data Analysis

1. Calculate the absorbance at 734 nm as percentage of the absorbance of the uninhibited radical cation solution (Blank) according to the equation:

$$\text{Inhibition of } A_{734\text{nm}} (\%) = (1 - (A_f/A_0)) \times 100$$

Where A_0 is the absorbance of uninhibited radical cation and A_f is, the absorbance measured 5 min after the addition of antioxidant samples.

2. Plot the inhibition of $A_{734\text{nm}}$ of standards as function of their final concentrations (Table 1). See Figure 2 for a typical standard curve.
3. Calculate the CEAC value of the samples using the equation obtained from the linear regression of the standard curve substituted of $A_{734\text{nm}}$ values for each sample.

$$\text{CEAC } (\mu\text{M}) = (\text{sample inhibition } A_{734\text{nm}} - \text{intercept}) / \text{slope}$$

Data Analysis

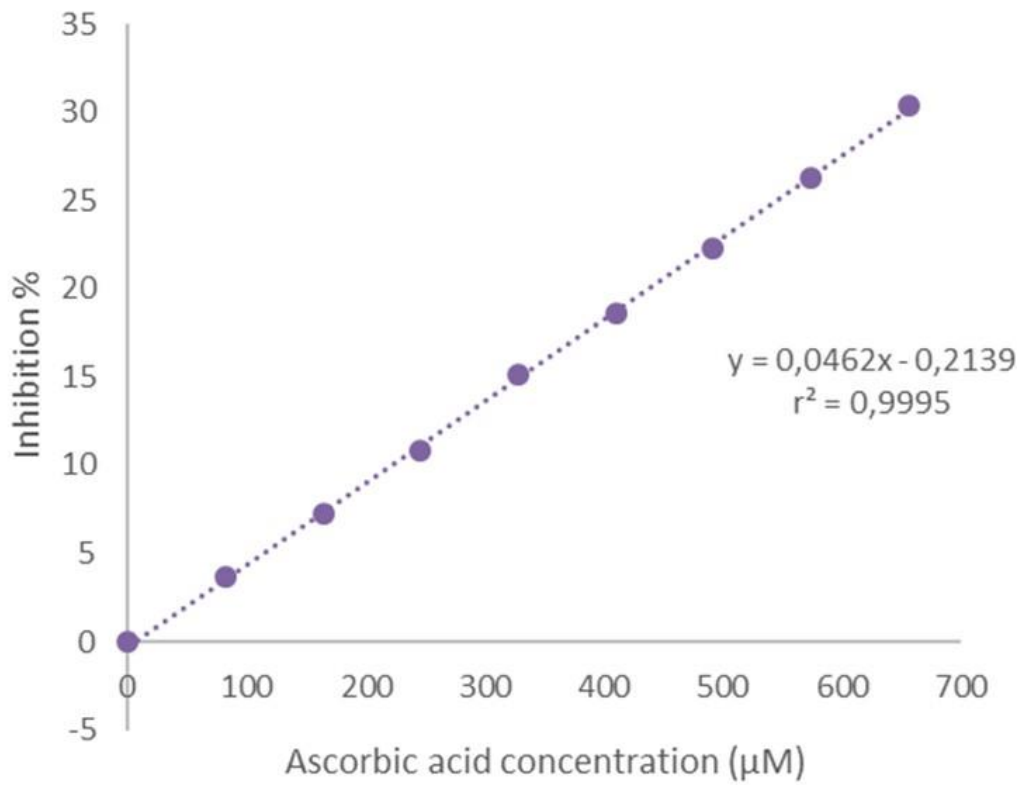


Figure 2. Typical standard curve for ABTS assay

Warranties and Limitation of Liability

Our partner Bioquochem shall not in any event be liable for incidental, consequential or special damages of any kind resulting from any use or failure of the products, even if Bioquochem has been advised of the possibility of such damage including, without limitation, liability for loss of use, loss of work in progress, down time, loss of revenue or profits, failure to realize savings, loss of products of buyer or other use or any liability of buyer to a third party on account of such loss, or for any labor or any other expense, damage or loss occasioned by such product including personal injury or property damage is caused by Bioquochem's gross negligence. All liability of Bioquochem hereunder shall be limited to the amounts paid by buyer for product. Buyer's exclusive remedy and Bioquochem's sole liability hereunder shall be limited to a refund of the purchase price, or the replacement of all material that does not meet our specifications. Said refund or replacement is conditioned on buyer giving written notice to Bioquochem within 30 days after arrival of the material at its destination.

Expiration date: 2 months from the date of delivery.

Votre interlocuteur en France, Belgique, Luxembourg et Suisse :

LIBIOS

83, rue Edmond Michelet - 69490 Pontcharra Sur Turdine - France

Tél. : +33 (0)4 74 13 03 02 - Fax : +33 (0)4 74 05 28 25 –

Mail : info@libios.fr - www.libios.fr