




CELLOPENTAOSE (Lot 180405)

O-CPE-20MG

09/18

MW: 828.72
CAS: 2240-27-9

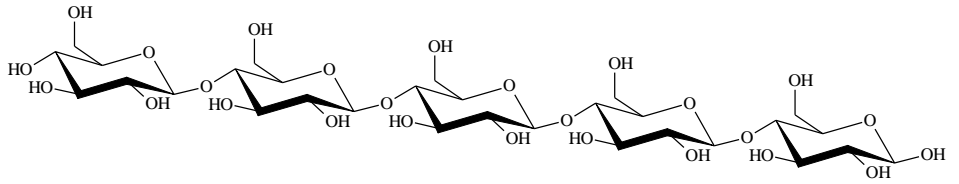

PREPARATION:

Prepared by controlled acid hydrolysis of cellulose acetate.

PURITY: > 95%

HPLC:


Column: 2 x Tosoh TSK-GEL G2500 PWXL (7.8 x 300 mm) plus guard column (7.8 x 35mm)

Temperature: 80°C

Mobile phase: dH₂O

Flow rate: 0.5 mL/min

HPLC System: Waters Alliance e2695 Separations Module, Waters 2414 RI detector and Empower v 3 software

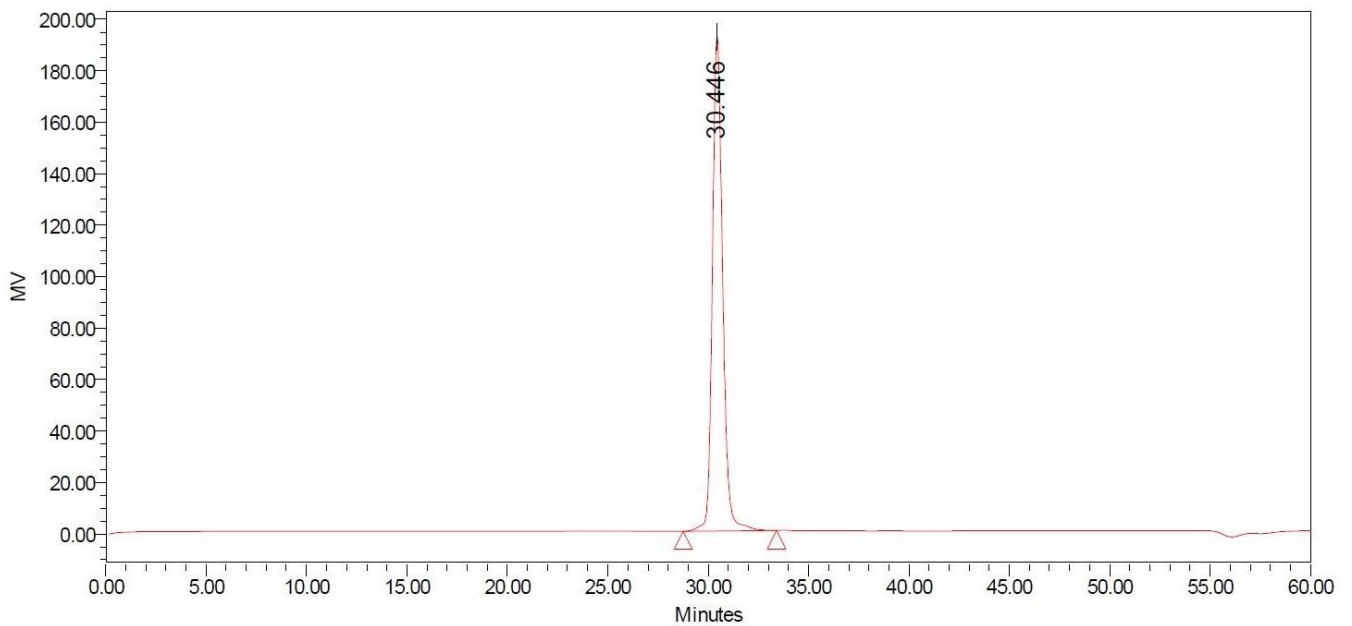

Peak Name:

	Injection	RT	Area	% Area	Height
1	1	30.446	6827598	100.00	192091

HPAEC-PAD:

Column: CarboPac PA200 guard and analytical columns (3 x 250 mm)

Temperature: 20°C

Detector: Au electrode; waveform Carbohydrate, standard quad

Flow rate: 0.4 mL/min

IC system: Dionex ICS5000+ DP system and Chromeleon 7 software

A stepwise linear gradient method was employed as shown.

Time (min)	100 mM NaOH (%)	120 mM NaOAc (%)
0	100	0
4	100	0
5	80	20
8	65	35
21	50	50
23	0	100
26	0	100
27	100	0
30	100	0

